



ZEAL INTERNATIONAL (An ISO 9001 Certified Company)

Head Office: 1, Netaji Subhash Marg Daryaganj, New Delhi - 110002 INDIA

Phone: +91-11-23276114, 23244474, 23250281, 23278846 Fax: +91-11-43580558

Branch Office: 4/20 Kirti Nagar Industrial Area New Delhi - 110015 Phone: +91 11 45380800

Warehouse: 4/26 Kirti Nagar Industrial Area New Delhi - 110015

info@zealinternational.com

sales@zealinternational.com

support@zealinternational.com

quotation@zealinternational.com


Visit us at: www.zealinternational.com

Laboratory Vane Shear Apparatus (Motorised) ZI 3076

Standards:

Specification:

Consists of a torque head adjustable in height by means of a lead screw rotated by a drive wheel to enable the vane to be lowered into the specimen. Rotation of the vane is by means of an electrically operated rate of rotating is 1/60 R.P.M. Suitable for operation on 230 V A.C. Single Phase which operates a worm gear arrangement turning the upper end of a calibration torsion spring, vane dia, rod dia, vane size & vane height are as per IS specifications.

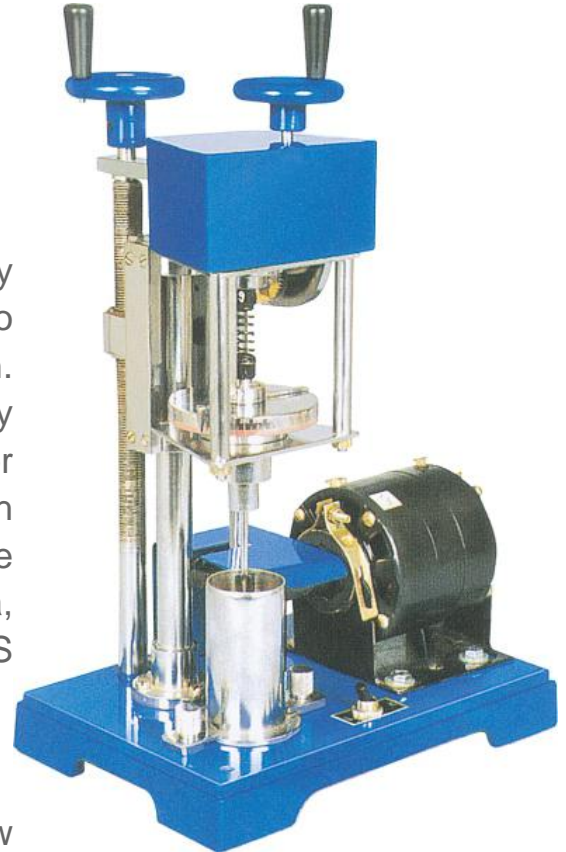

The vane shaft is attached through the hollow upper shaft to a resettable pointer, which indicates the angle indicates the angle of torque on a dial graduated in degree the dial reading multiplied by spring factor gives the torque a container for soil sample is also supplied & a sampling tube of 38mm. i.d. & 150mm long can also be used as container . Supplied with set of four springs, one each of approx. 2 kgs/cm², 4kgs/cm², 6 kgs/cm² & 8kgs/cm² complete as above in a wooden carrying case.